


RAYON X DIFFRACTION

d'echantillon	N DSX4 LIPTAKO NIGRA
Target/Filter	Cu / Monochromator
Voltage/Current	40 KV / 30mA
Count Full Scale	800 cps
Time Constant	2 sec.
Slit System	1-1-0.15mm-0.45mm
Scan Speed	2 deg/min.
Chart Speed	20mm/min


SUMIKO CONSULTANTS CO., LTD.


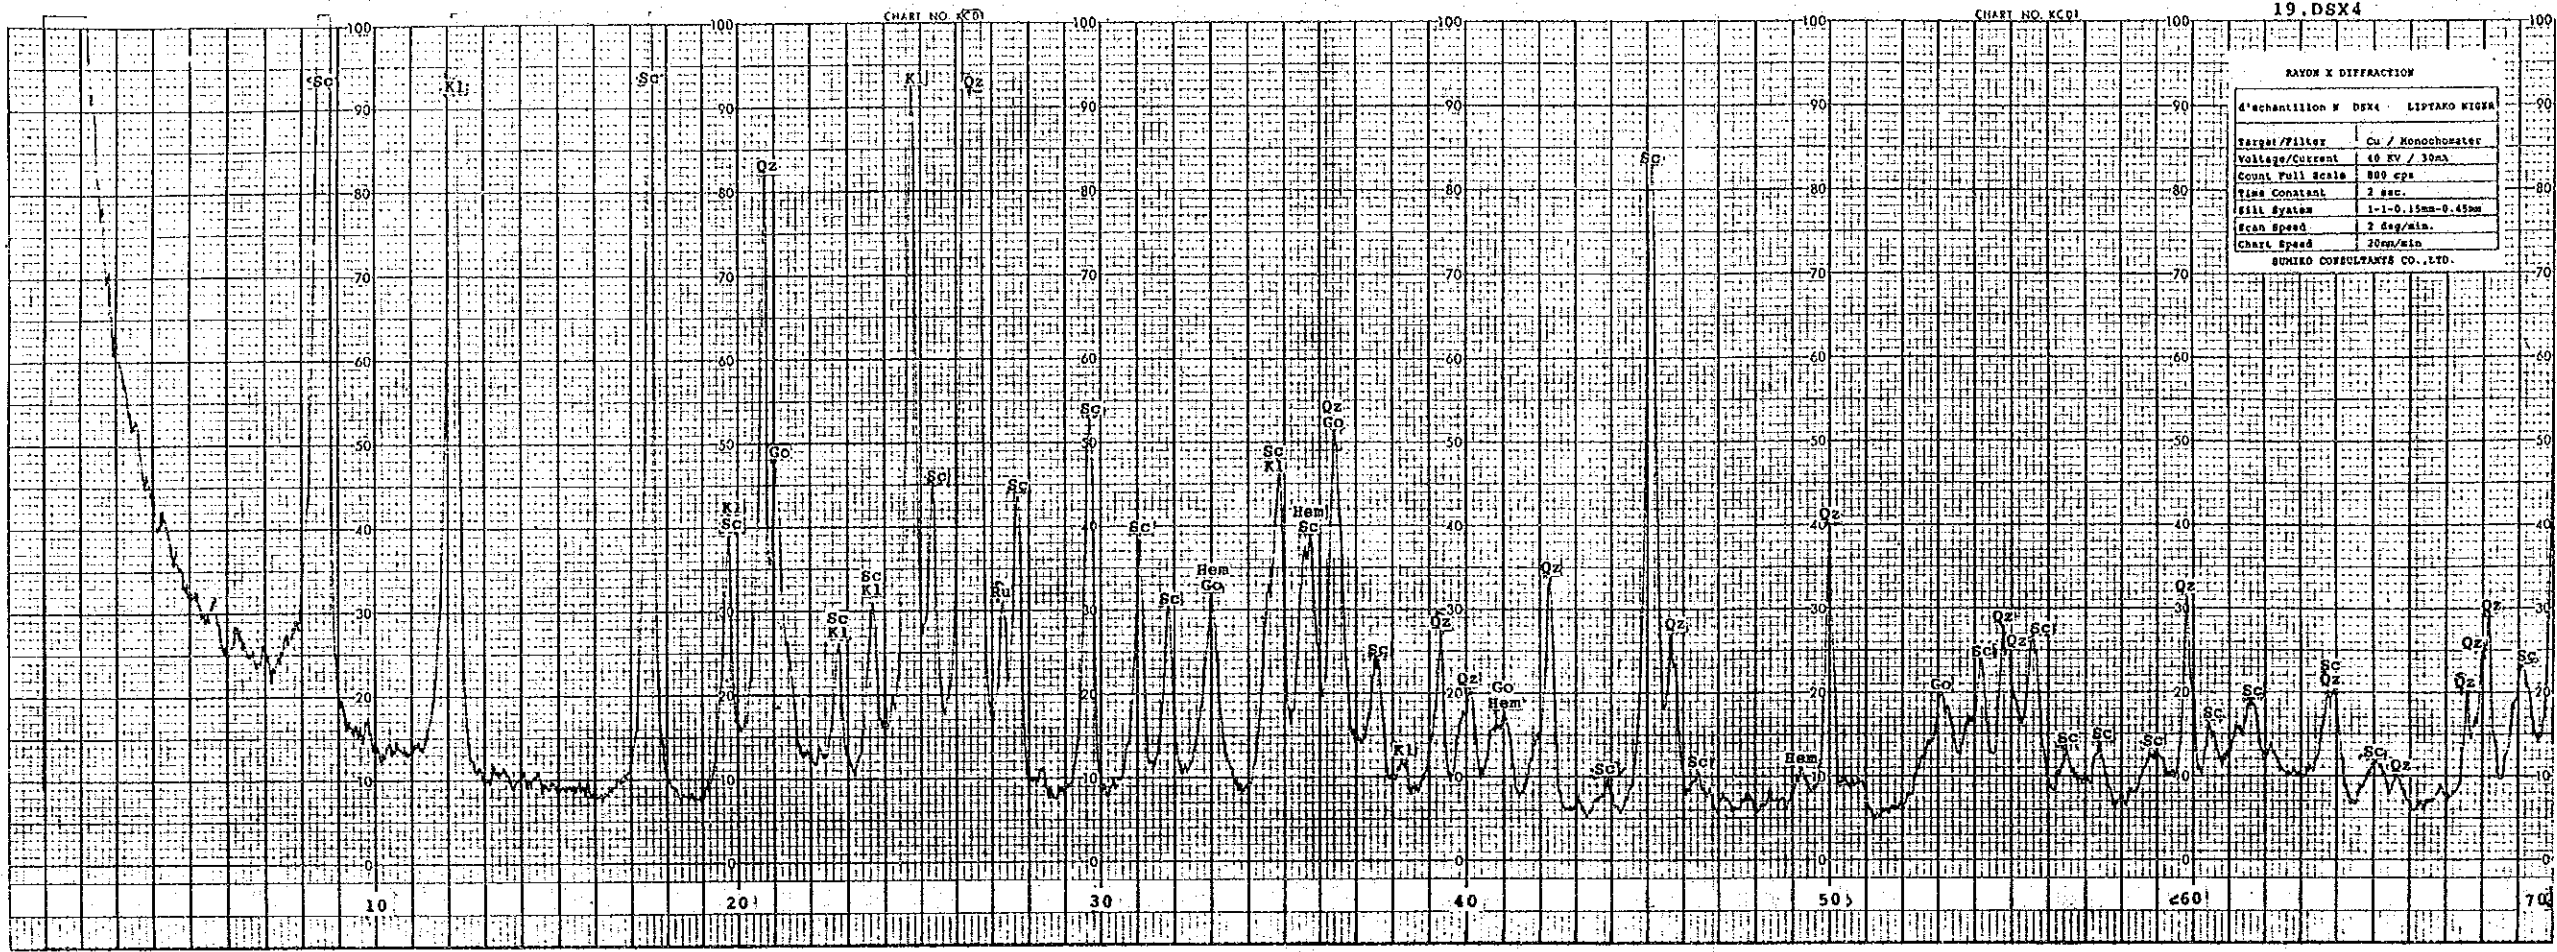




RAYON X DIFFRACTION



d'echantillon	N DSX5 LIPTAKO NIGRA
Target/Filter	Cu / Monochromator
Voltage/Current	40 KV / 30mA
Count Full Scale	800 cps
Time Constant	2 sec.
Slit System	1-1-0.15mm-0.45mm
Scan Speed	2 deg/min.
Chart Speed	20mm/min

SUMIKO CONSULTANTS CO., LTD.

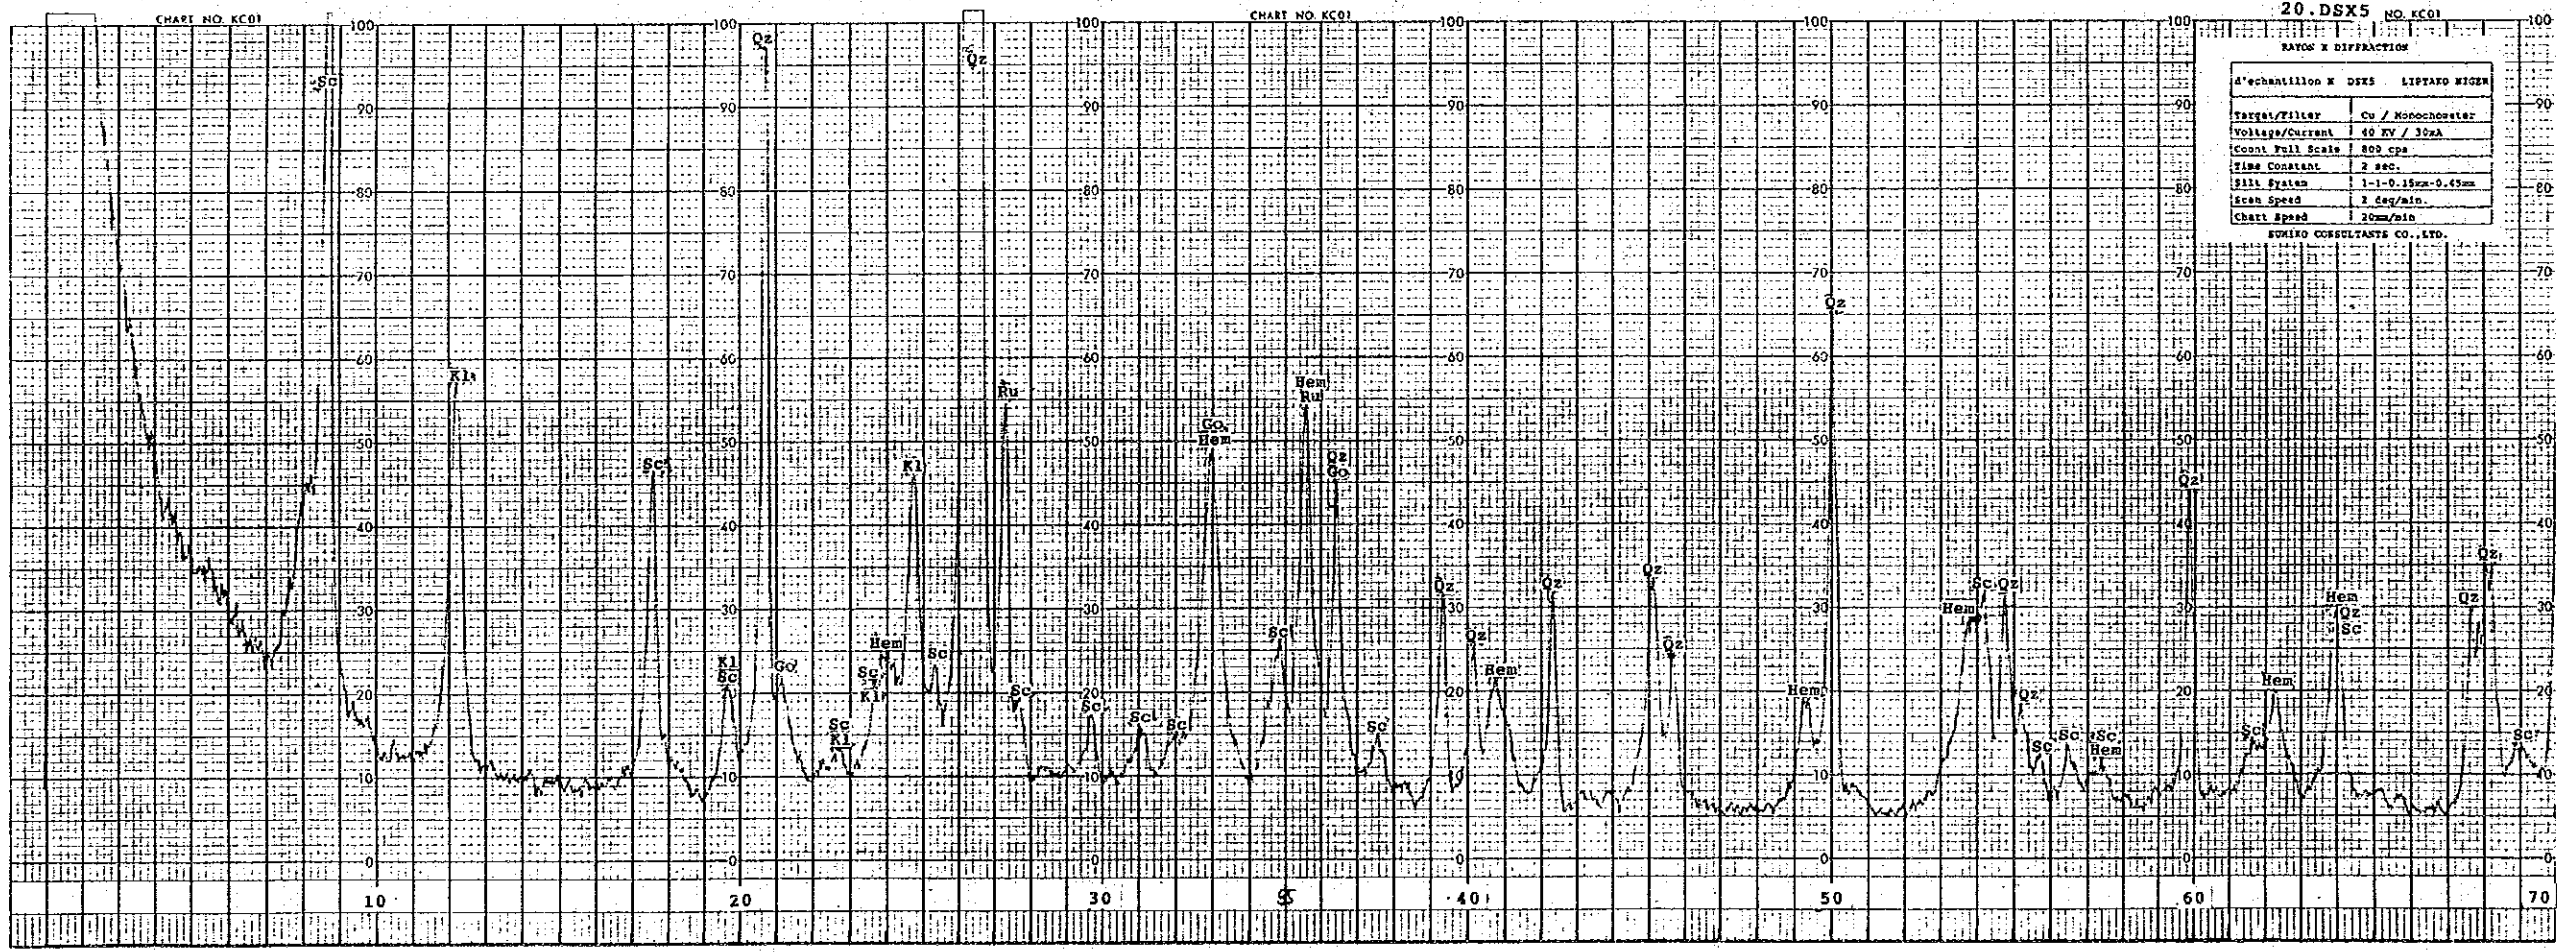

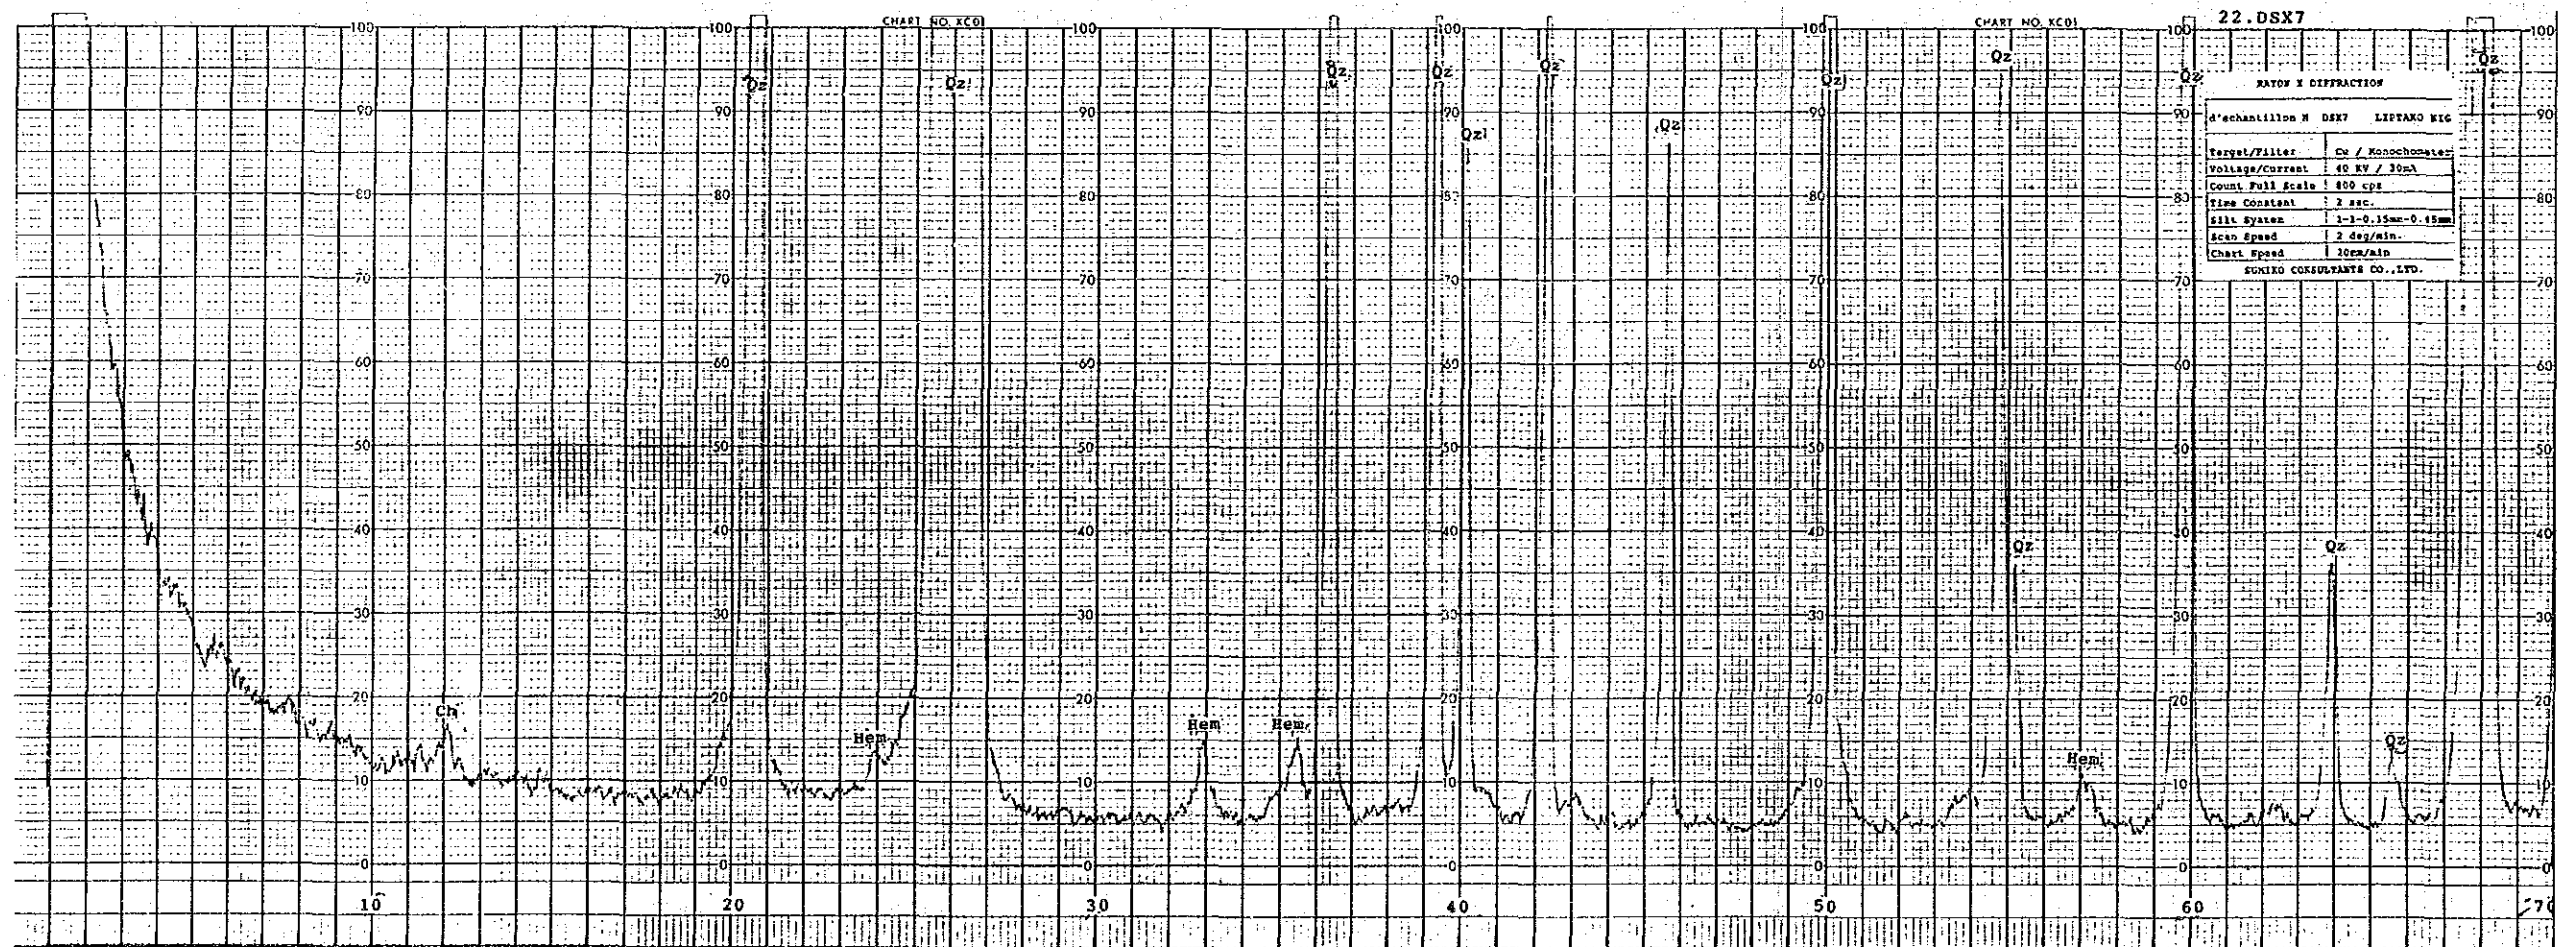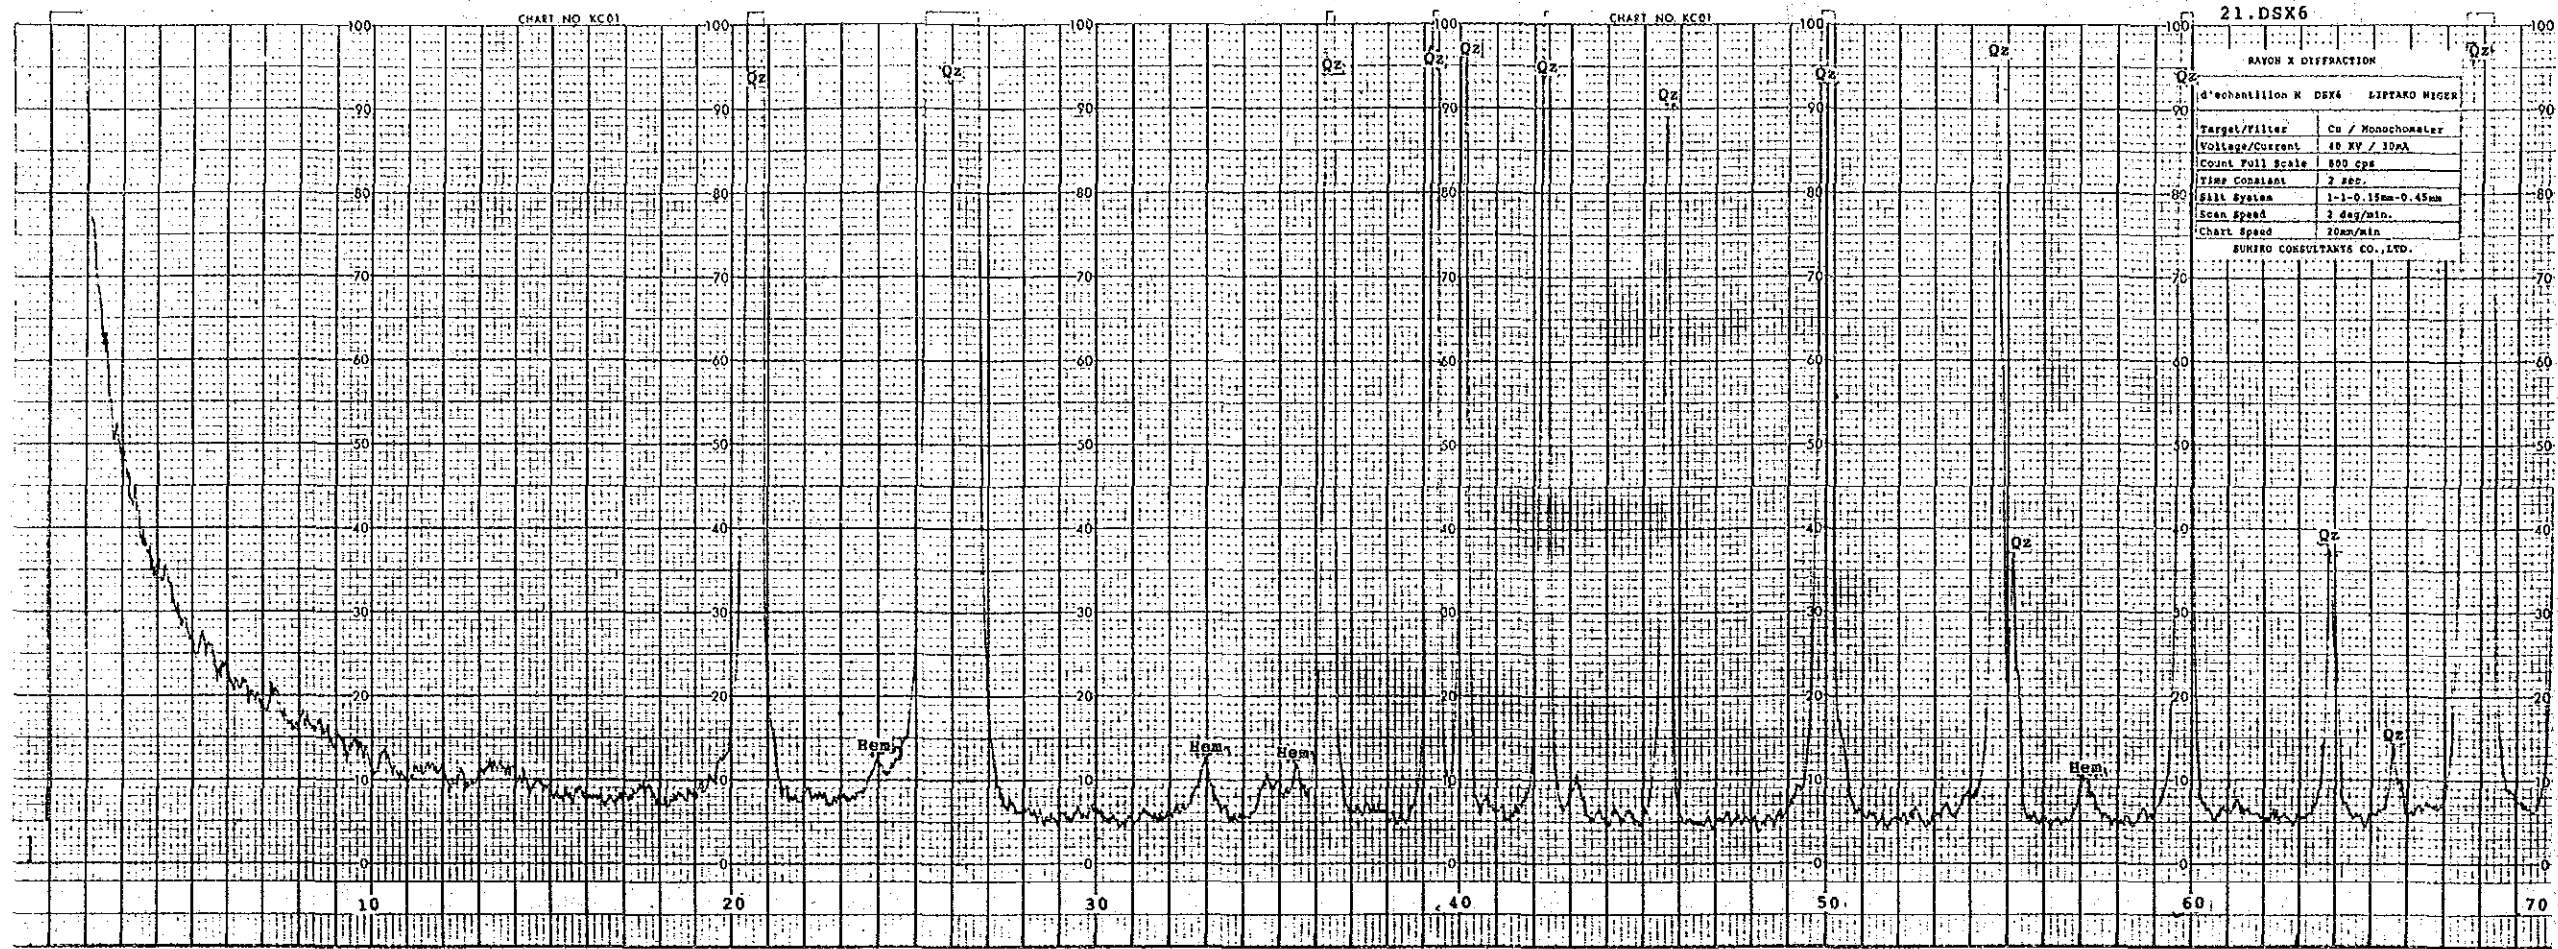


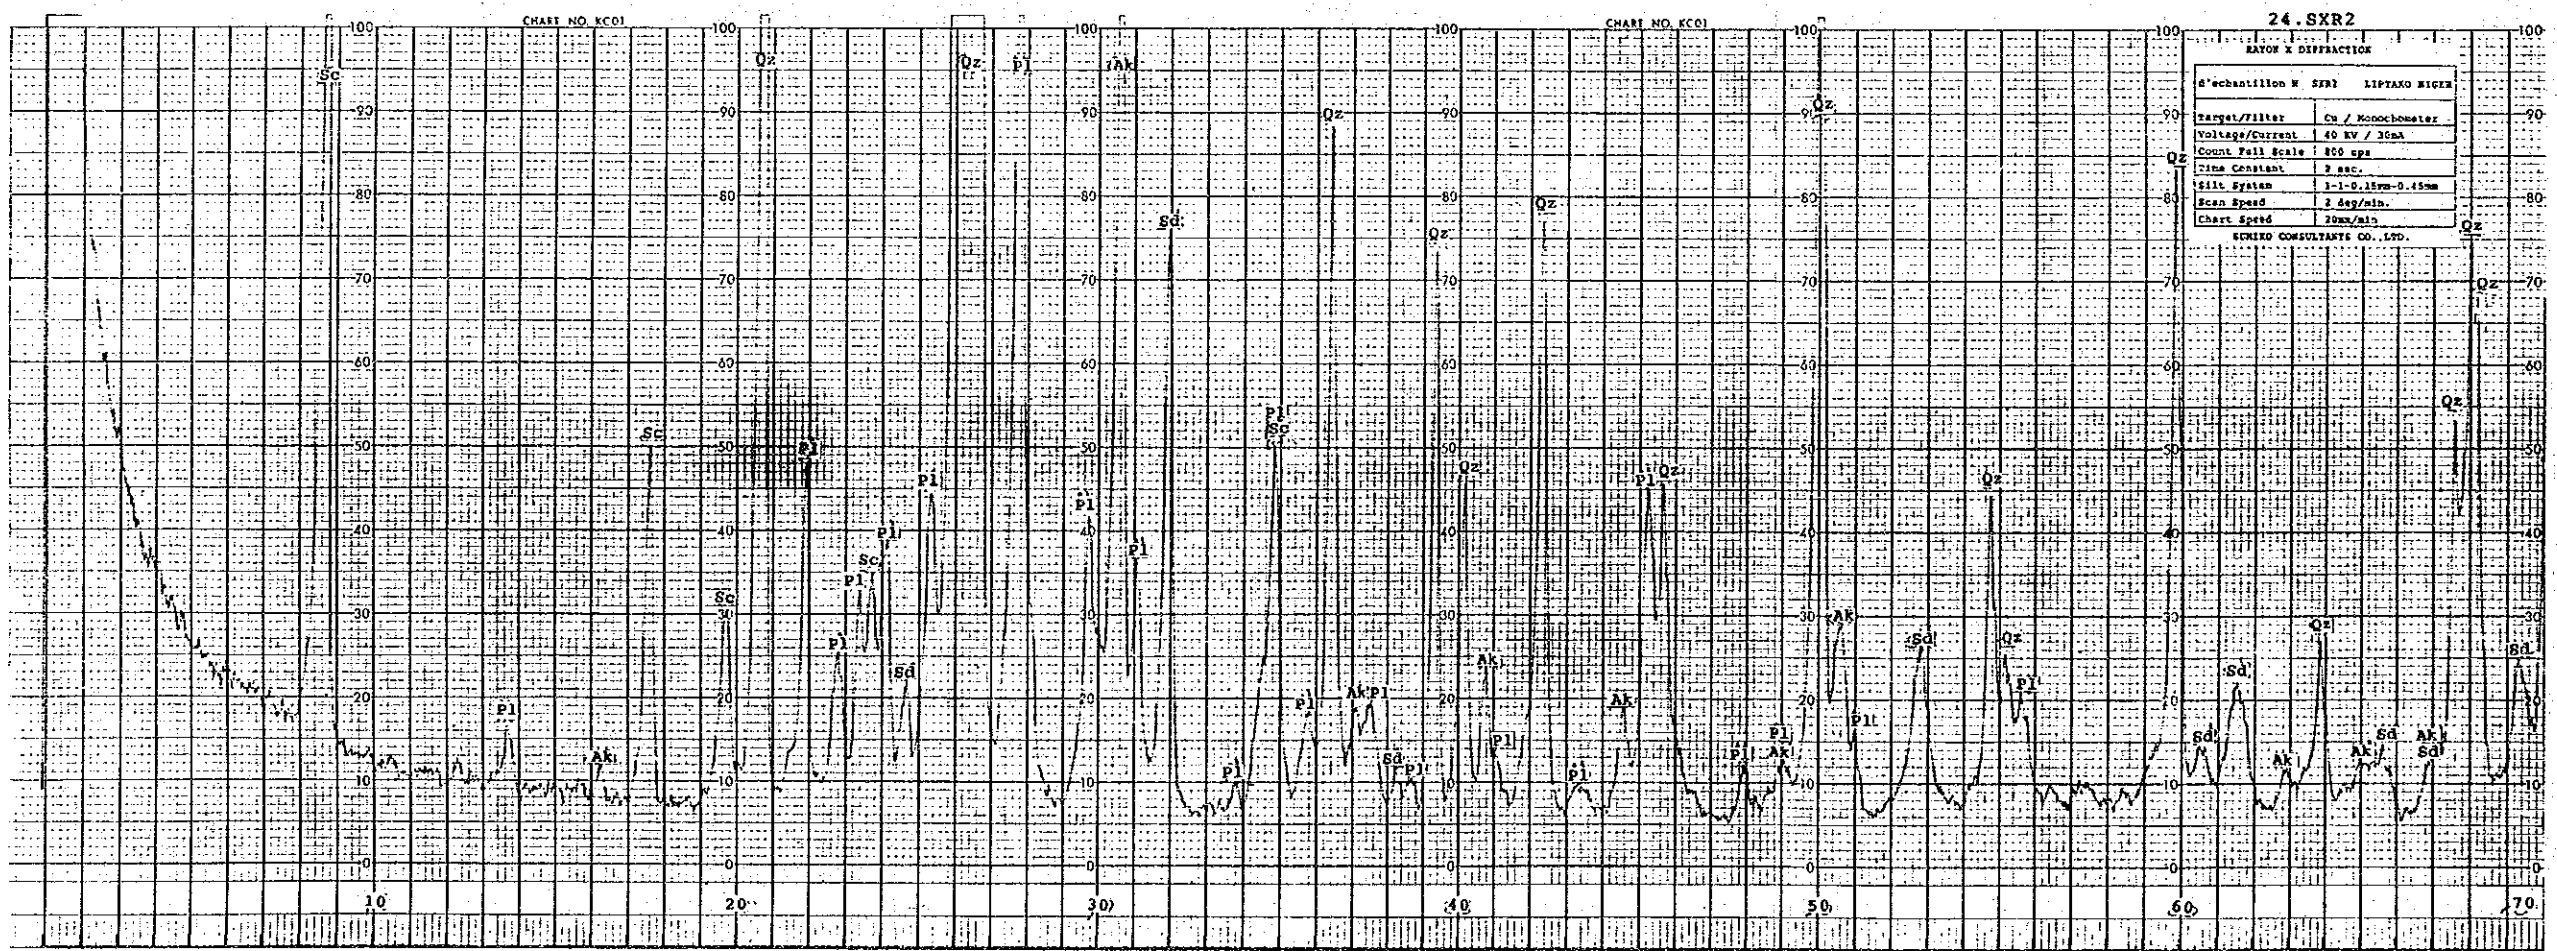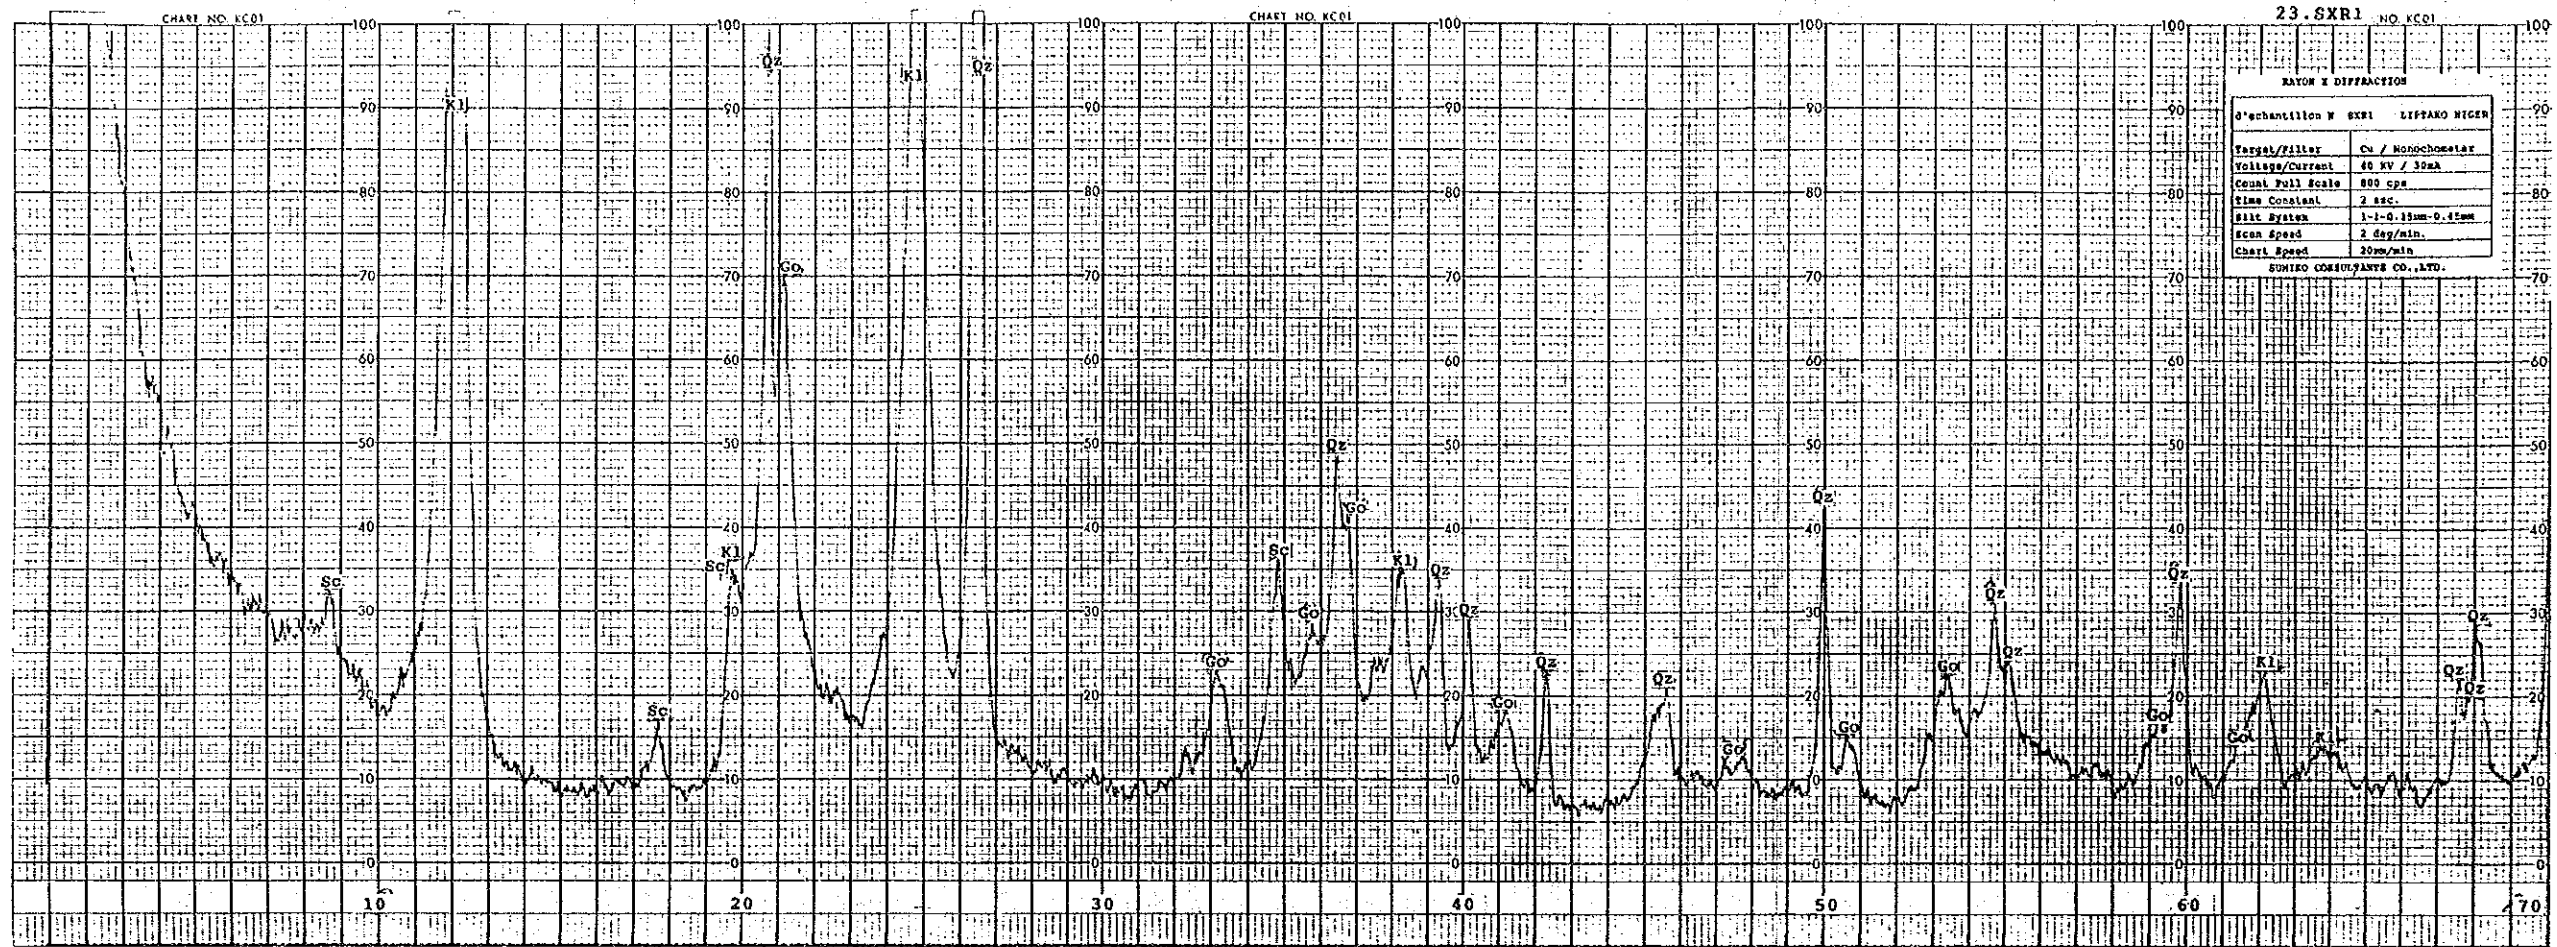

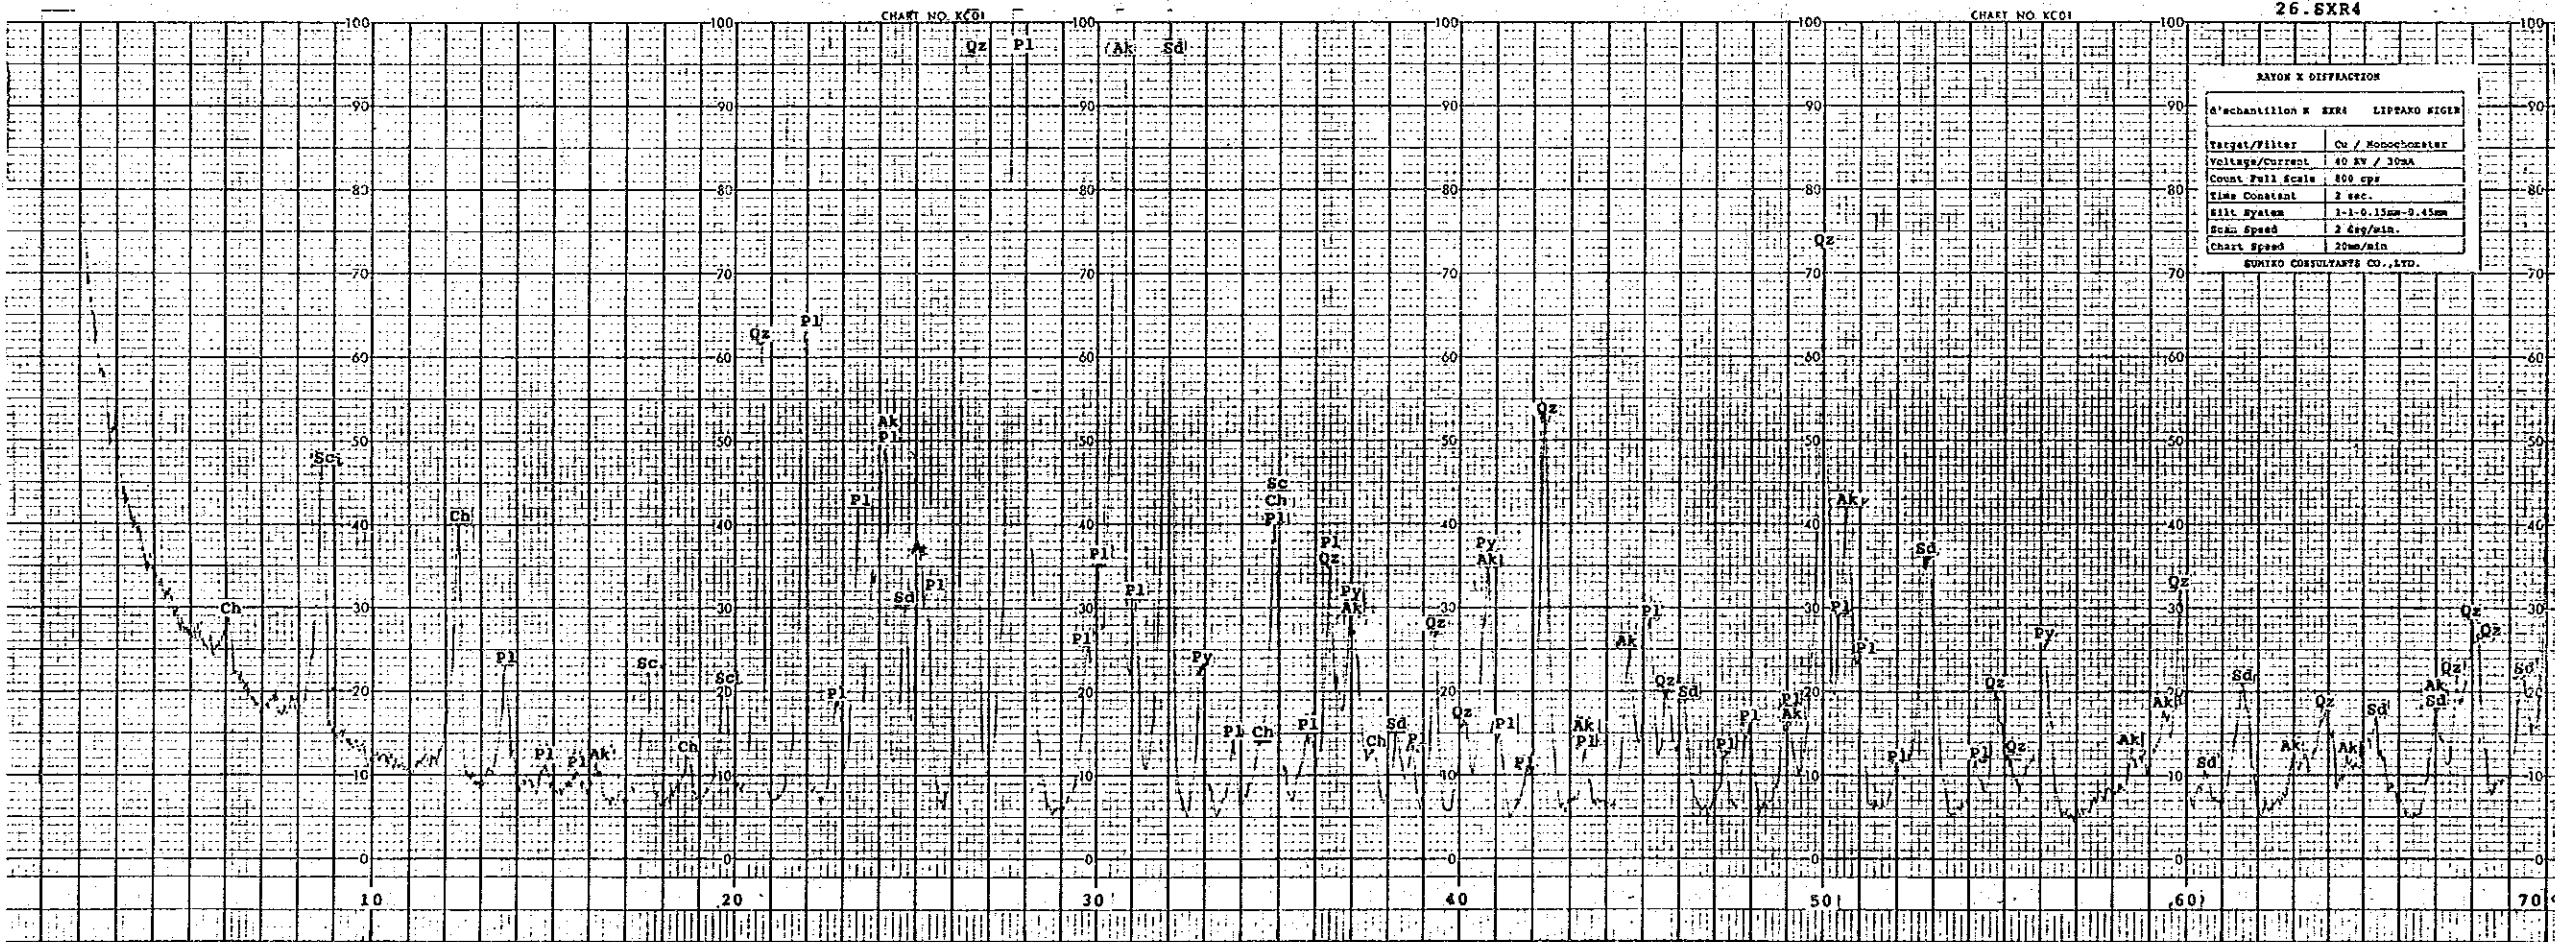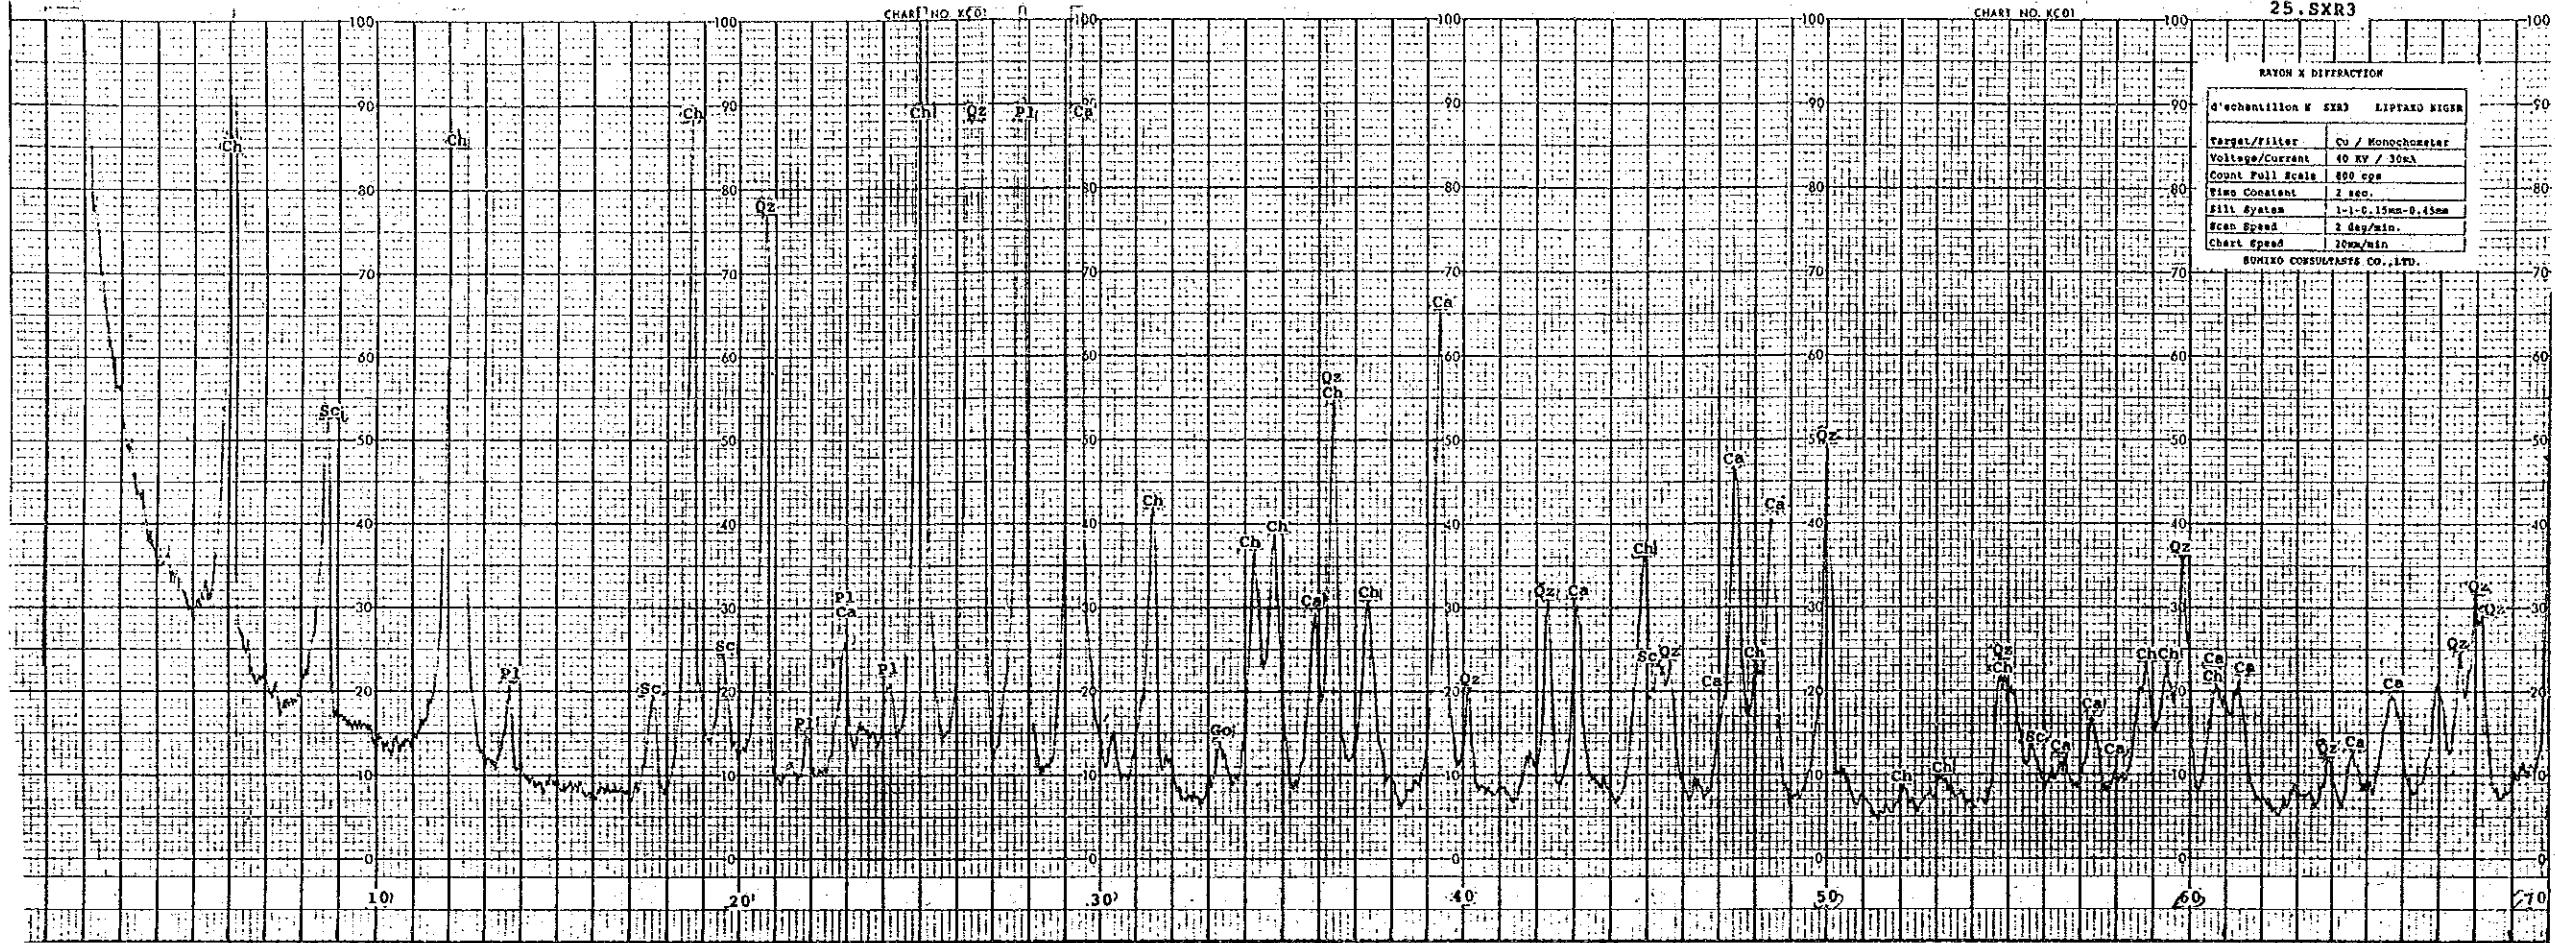

27. SXR5 NO. KC01

RAYON X DIFFRACTION	
d'schabillon #	SXR5 LIPTAKO NIGER
Target/Filter	Cu / Monochromator
Voltage/Current	40 KV / 30mA
Count Full Scale	600 cps
Time Constant	2 sec.
Slit System	1-1-0.15mm-0.45mm
Scan Speed	2 deg/min.
Chart Speed	20mm/min.
SUMIKO CONSULTANTS CO., LTD.	

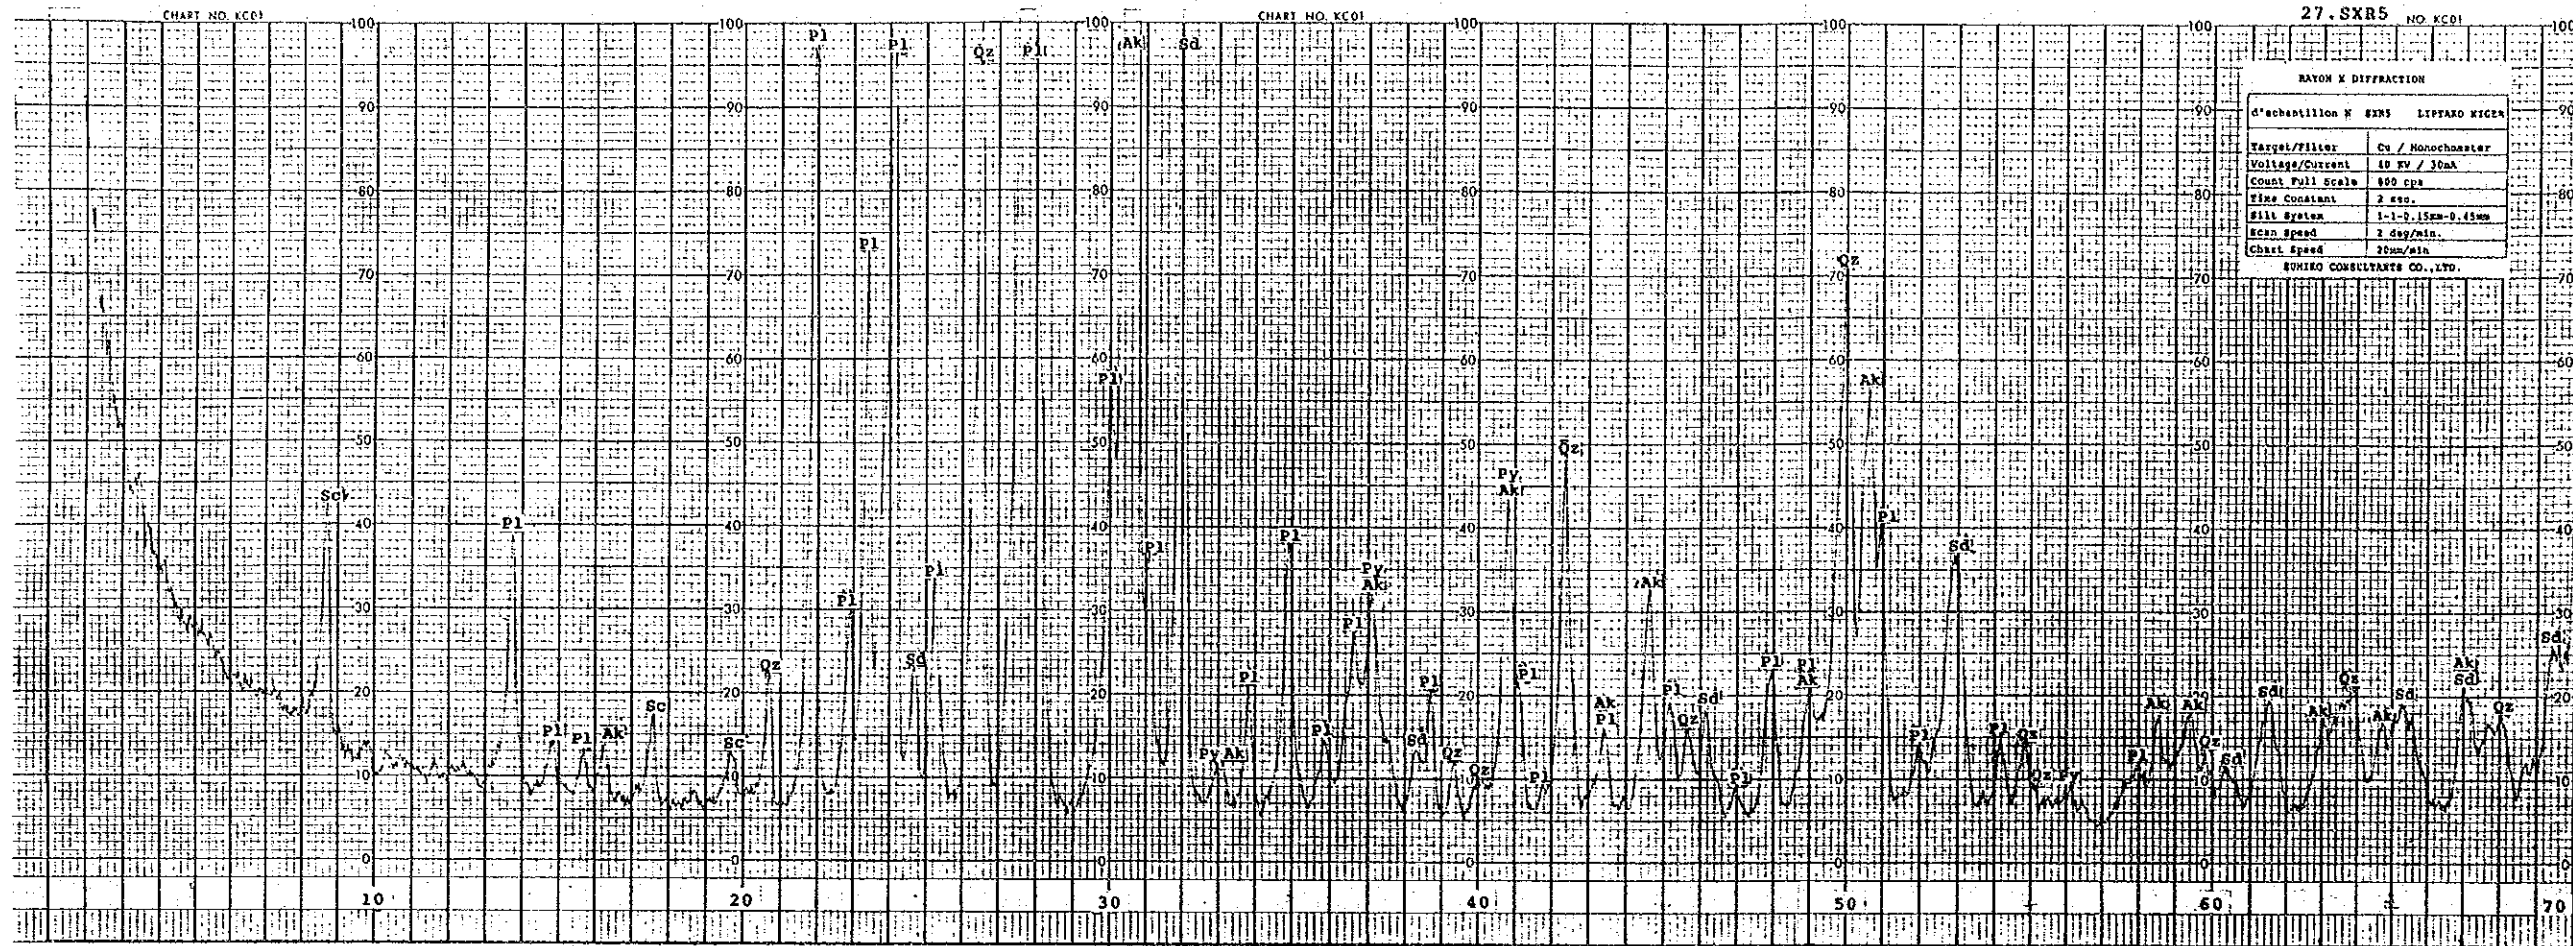

28. SXR6

RAYON X DIFFRACTION	
d'schabillon #	SXR6 LIPTAKO NIGER
Target/Filter	Cu / Monochromator
Voltage/Current	40 KV / 30mA
Count Full Scale	600 cps
Time Constant	2 sec.
Slit System	1-1-0.15mm-0.45mm
Scan Speed	2 deg/min.
Chart Speed	20mm/min.
SUMIKO CONSULTANTS CO., LTD.	

